



US008558563B2

(12) **United States Patent**  
**Zdeblick**

(10) **Patent No.:** **US 8,558,563 B2**

(45) **Date of Patent:** **Oct. 15, 2013**

(54) **APPARATUS AND METHOD FOR MEASURING BIOCHEMICAL PARAMETERS**

(75) Inventor: **Mark J. Zdeblick**, Portola Valley, CA (US)

(73) Assignee: **Proteus Digital Health, Inc.**, Redwood City, CA (US)

(\* ) Notice: Subject to any disclaimer, the term of this patent is extended or adjusted under 35 U.S.C. 154(b) by 0 days.

(21) Appl. No.: **13/390,866**

(22) PCT Filed: **Aug. 23, 2010**

(86) PCT No.: **PCT/US2010/046381**

§ 371 (c)(1),  
(2), (4) Date: **Feb. 16, 2012**

(87) PCT Pub. No.: **WO2011/022732**

PCT Pub. Date: **Feb. 24, 2011**

(65) **Prior Publication Data**

US 2012/0146670 A1 Jun. 14, 2012

**Related U.S. Application Data**

(60) Provisional application No. 61/235,979, filed on Aug. 21, 2009.

(51) **Int. Cl.**  
**G01R 27/08** (2006.01)  
**A61B 5/053** (2006.01)

(52) **U.S. Cl.**  
USPC ..... **324/692; 600/547**

(58) **Field of Classification Search**  
USPC ..... **324/692, 691, 649, 600**  
See application file for complete search history.

(56) **References Cited**

**U.S. PATENT DOCUMENTS**

3,589,943 A 6/1971 Grubb et al.  
3,607,788 A 9/1971 Adolph

(Continued)

**FOREIGN PATENT DOCUMENTS**

EP 0344939 12/1989  
EP 1246356 10/2002

(Continued)

**OTHER PUBLICATIONS**

AADE, "AADE 37th Annual Meeting San Antonio Aug. 4-7, 2010" American Association of Diabetes Educators (2010); <http://www.diabeteseducator.org/annualmeeting/2010/index.html>; 2 pp.

(Continued)


*Primary Examiner* — Hoai-An D Nguyen

(74) *Attorney, Agent, or Firm* — Oppedahl Patent Law Firm LLC

(57) **ABSTRACT**

In a first embodiment, electrodes are coupled to a surface at first, second, and third locations, the first location being further from the third location than from the second location. Impedance is measured at distinct frequencies between pairs of the electrodes. As a result, impedance is measured at differing regions below the surface, one region being deeper below the surface than the other region. In a second embodiment, a microfluidic device carries out an analysis. The analysis may be within a flexible patch adhered to a surface, or may be in a solid device implanted in a body of liquid surrounded by tissue. The analysis may involve pumping a fluid or may involve drawing an analyte electrophoretically through a microfluidic channel.

**9 Claims, 2 Drawing Sheets**

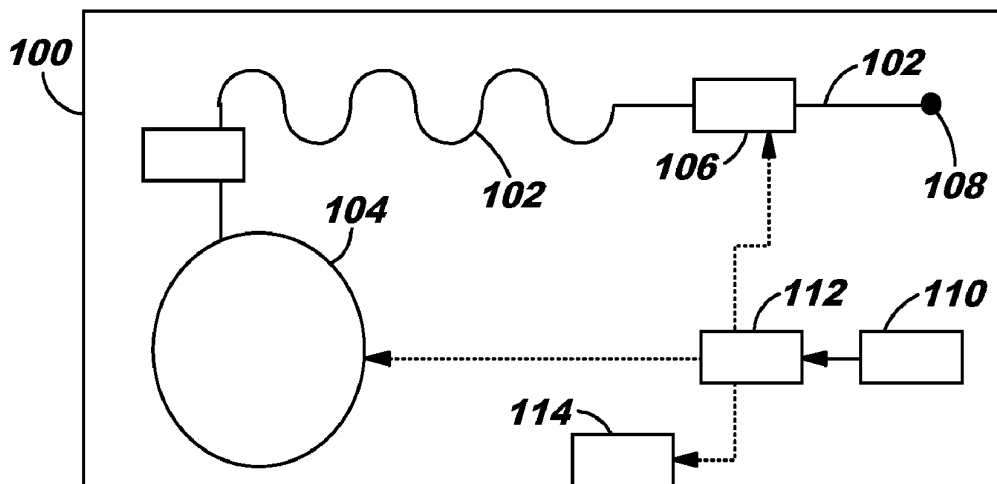

(56)

References Cited

U.S. PATENT DOCUMENTS

3,642,008 A	2/1972	Bolduc	5,957,854 A	9/1999	Besson et al.
3,679,480 A	7/1972	Brown et al.	5,963,132 A	10/1999	Yoakum et al.
3,682,160 A	8/1972	Murata	5,974,124 A	10/1999	Schlueter, Jr. et al.
3,719,183 A	3/1973	Schwartz	5,981,166 A	11/1999	Mandecki
3,799,802 A	3/1974	Schneble, Jr. et al.	5,999,846 A	12/1999	Pardey et al.
3,828,766 A	8/1974	Krasnow	6,038,464 A	3/2000	Axelgaard et al.
3,837,339 A	9/1974	Aisenberg et al.	6,042,710 A	3/2000	Dubrow
3,893,111 A	7/1975	Cotter	6,047,203 A	4/2000	Sackner
3,967,202 A	6/1976	Batz	6,076,016 A	6/2000	Feierbach et al.
3,989,050 A	11/1976	Buchalter	6,081,734 A	6/2000	Batz
4,017,856 A	4/1977	Wiegand	6,091,975 A	7/2000	Daddona et al.
4,055,178 A	10/1977	Harrigan	6,095,985 A	8/2000	Raymond et al.
4,077,397 A	3/1978	Ellis	6,115,636 A	9/2000	Ryan
4,077,398 A	3/1978	Ellis	6,122,351 A	9/2000	Schlueter, Jr. et al.
4,082,087 A	4/1978	Howson	6,141,592 A	10/2000	Pauly
4,090,752 A	5/1978	Long	6,200,265 B1	3/2001	Walsh et al.
4,106,348 A	8/1978	Auphan	6,206,702 B1	3/2001	Hayden et al.
4,129,125 A	12/1978	Lester	6,217,744 B1	4/2001	Crosby
4,166,453 A	9/1979	McClelland	6,231,593 B1	5/2001	Meserol
4,239,046 A	12/1980	Ong	6,245,057 B1	6/2001	Sieben et al.
4,251,795 A *	2/1981	Shibasaki et al. ....	6,269,058 B1	7/2001	Yamanoi et al.
4,269,189 A	5/1981	Abraham	6,285,897 B1	9/2001	Kilcoyne et al.
4,331,654 A	5/1982	Morris	6,287,252 B1	9/2001	Lugo
4,345,588 A	8/1982	Widder et al.	6,288,629 B1	9/2001	Cofino et al.
4,418,697 A	12/1983	Tama	6,289,238 B1	9/2001	Besson et al.
4,425,117 A	1/1984	Hugemann	6,315,719 B1	11/2001	Rode et al.
4,494,950 A	1/1985	Fischell	6,342,774 B1	1/2002	Kreisinger et al.
4,559,950 A	12/1985	Vaughan	6,358,202 B1	3/2002	Arent
4,635,641 A	1/1987	Hoffman	6,364,834 B1	4/2002	Reuss
4,654,165 A	3/1987	Eisenber	6,366,206 B1	4/2002	Ishikawa et al.
4,663,250 A	5/1987	Ong et al.	6,368,190 B1	4/2002	Easter et al.
4,669,479 A	6/1987	Dunseath	6,371,927 B1	4/2002	Brune
4,725,997 A	2/1988	Urquhart et al.	6,374,670 B1	4/2002	Spelman
4,763,659 A	8/1988	Dunseath	6,380,858 B1	4/2002	Yarin et al.
4,767,627 A	8/1988	Caldwell et al.	6,394,997 B1	5/2002	Lemelson
4,784,162 A	11/1988	Ricks	6,426,863 B1	7/2002	Munshi
4,793,825 A	12/1988	Benjamin	6,432,292 B1	8/2002	Pinto et al.
4,844,076 A	7/1989	Lesho	6,440,069 B1	8/2002	Raymond et al.
4,896,261 A	1/1990	Nolan	6,441,747 B1	8/2002	Khair
4,975,230 A	12/1990	Pinkhasov	6,453,199 B1	9/2002	Kobozev
4,987,897 A	1/1991	Funke	6,477,424 B1	11/2002	Thompson et al.
5,016,634 A	5/1991	Vock et al.	6,496,705 B1	12/2002	Ng et al.
5,079,006 A	1/1992	Urquhart	6,526,315 B1	2/2003	Inagawa
5,167,626 A	12/1992	Casper	6,531,026 B1	3/2003	Takeichi et al.
5,176,626 A	1/1993	Soehendra	6,544,174 B2	4/2003	West
5,261,402 A	11/1993	DiSabito	6,564,079 B1	5/2003	Cory
5,263,481 A	11/1993	Axelgaard et al.	6,572,636 B1	6/2003	Hagen et al.
5,279,607 A	1/1994	Schentag et al.	6,577,893 B1	6/2003	Besson et al.
5,281,287 A	1/1994	Lloyd	6,579,231 B1	6/2003	Phipps
5,283,136 A	2/1994	Peled et al.	6,595,929 B2	7/2003	Stivoric
5,305,745 A *	4/1994	Zacouto .....	6,605,038 B1	8/2003	Teller
5,318,557 A	6/1994	Gross	6,609,018 B2	8/2003	Cory
5,394,882 A	3/1995	Mawhinney	6,612,984 B1	9/2003	Kerr
5,395,366 A	3/1995	D'Andrea et al.	6,632,175 B1	10/2003	Marshall
5,436,091 A	7/1995	Shackle et al.	6,632,216 B2	10/2003	Houzeago et al.
5,443,461 A	8/1995	Atkinson et al.	6,635,279 B2	10/2003	Kolter et al.
5,443,843 A	8/1995	Curatolo et al.	6,643,541 B2	11/2003	Mok et al.
5,458,141 A	10/1995	Neil et al.	6,654,638 B1	11/2003	Sweeney
5,485,841 A	1/1996	Watkin et al.	6,663,846 B1	12/2003	McCombs
5,567,210 A	10/1996	Bates et al.	6,673,474 B2	1/2004	Yamamoto
5,596,302 A	1/1997	Mastrocola et al.	6,680,923 B1	1/2004	Leon
5,600,548 A	2/1997	Nguyen et al.	6,689,117 B2	2/2004	Sweeney et al.
5,634,468 A	6/1997	Platt	6,694,161 B2	2/2004	Mehrotra
5,645,063 A	7/1997	Straka et al.	6,704,602 B2	3/2004	Berg et al.
5,705,189 A	1/1998	Lehmann et al.	6,720,923 B1	4/2004	Hayward et al.
5,738,708 A	4/1998	Peachey et al.	6,738,671 B2	5/2004	Christophersom et al.
5,740,811 A	4/1998	Hedberg	6,740,033 B1	5/2004	Olejniczak et al.
5,757,326 A	5/1998	Koyama et al.	6,745,082 B2	6/2004	Axelgaard et al.
5,792,048 A	8/1998	Schaefer	6,755,783 B2	6/2004	Cosentino
5,802,467 A	9/1998	Salazar	6,757,523 B2	6/2004	Fry
5,833,716 A	11/1998	Bar-Or	6,759,968 B2	7/2004	Zierolf
5,845,265 A	12/1998	Woolston	6,800,060 B2	10/2004	Marshall
5,862,803 A	1/1999	Besson	6,801,137 B2	10/2004	Eggers et al.
5,868,136 A	2/1999	Fox	6,822,554 B2	11/2004	Vrijens et al.
5,925,030 A	7/1999	Gross et al.	6,836,862 B1	12/2004	Erekson et al.
			6,839,659 B2	1/2005	Tarassenko et al.
			6,840,904 B2	1/2005	Goldberg
			6,842,636 B2	1/2005	Perrault
			6,845,272 B1	1/2005	Thomsen

(56)

## References Cited

## U.S. PATENT DOCUMENTS

6,864,780 B2	3/2005	Doi	7,376,435 B2	5/2008	McGowan
6,879,810 B2	4/2005	Bouet	7,382,263 B2	6/2008	Danowski et al.
6,909,878 B2	6/2005	Haller	7,387,607 B2	6/2008	Holt
6,922,592 B2	7/2005	Thompson et al.	7,388,903 B2	6/2008	Godfrey et al.
6,928,370 B2	8/2005	Anuzis et al.	7,389,088 B2	6/2008	Kim
6,929,636 B1	8/2005	Von Alten	7,392,015 B1	6/2008	Farlow
6,937,150 B2	8/2005	Medema	7,395,106 B2	7/2008	Ryu et al.
6,942,616 B2	9/2005	Kerr	7,396,330 B2	7/2008	Banet
6,951,536 B2	10/2005	Yokoi	7,404,968 B2	7/2008	Abrams et al.
6,957,107 B2	10/2005	Rogers et al.	7,413,544 B2	8/2008	Kerr
6,968,153 B1	11/2005	Heinonen	7,414,534 B1	8/2008	Kroll et al.
6,987,965 B2	1/2006	Ng et al.	7,414,543 B2	8/2008	Rye et al.
6,990,082 B1	1/2006	Zehavi et al.	7,415,242 B1	8/2008	Ngan
7,002,476 B2	2/2006	Rapchak	7,424,268 B2	9/2008	Diener
7,004,395 B2	2/2006	Koenck	7,424,319 B2	9/2008	Muehlsteff
7,009,634 B2	3/2006	Iddan et al.	7,427,266 B2	9/2008	Ayer et al.
7,009,946 B1	3/2006	Kardach	7,471,665 B2	12/2008	Perlman
7,013,162 B2	3/2006	Gorsuch	7,499,674 B2	3/2009	Salokannel
7,016,648 B2	3/2006	Haller	7,510,121 B2	3/2009	Koenck
7,020,508 B2	3/2006	Stivoric	7,512,448 B2	3/2009	Malick
7,024,248 B2	4/2006	Penner et al.	7,515,043 B2	4/2009	Welch
7,031,745 B2	4/2006	Shen	7,519,416 B2 *	4/2009	Sula et al. .... 600/509
7,031,857 B2	4/2006	Tarassenko et al.	7,523,756 B2	4/2009	Minai
7,039,453 B2	5/2006	Mullick	7,525,426 B2	4/2009	Edelstein
7,044,911 B2	5/2006	Drinan et al.	7,539,533 B2	5/2009	Tran
7,046,649 B2	5/2006	Awater et al.	7,542,878 B2	6/2009	Nanikashvili
7,118,531 B2	10/2006	Krill	7,551,590 B2	6/2009	Haller
7,127,300 B2	10/2006	Mazar et al.	7,554,452 B2	6/2009	Cole
7,146,228 B2	12/2006	Nielsen	7,575,005 B2	8/2009	Mumford
7,146,449 B2	12/2006	Do et al.	7,616,111 B2	11/2009	Covannon
7,149,581 B2	12/2006	Goedeke et al.	7,617,001 B2	11/2009	Penner et al.
7,154,071 B2	12/2006	Sattler et al.	7,639,473 B2	12/2009	Hsu et al.
7,155,232 B2	12/2006	Godfrey et al.	7,640,802 B2	1/2010	King et al.
7,160,258 B2	1/2007	Imran	7,647,112 B2	1/2010	Tracey
7,164,942 B2	1/2007	Avrahami	7,647,185 B2	1/2010	Tarassenko et al.
7,171,166 B2	1/2007	Ng et al.	7,653,031 B2	1/2010	Godfrey et al.
7,171,177 B2	1/2007	Park et al.	7,672,714 B2	3/2010	Kuo
7,171,259 B2	1/2007	Rytky	7,673,679 B2	3/2010	Harrison et al.
7,176,784 B2	2/2007	Gilbert et al.	7,678,043 B2	3/2010	Gilad
7,187,960 B2	3/2007	Abreu	7,697,994 B2	4/2010	VanDanacker et al.
7,188,767 B2	3/2007	Penuela	7,720,036 B2	5/2010	Sadri
7,194,038 B1	3/2007	Inkinen	7,729,776 B2	6/2010	Von Arx et al.
7,206,630 B1	4/2007	Tarler	7,733,224 B2	6/2010	Tran
7,209,790 B2	4/2007	Thompson et al.	7,736,318 B2	6/2010	Costentino
7,215,660 B2	5/2007	Perlman	7,756,587 B2	7/2010	Penner et al.
7,215,991 B2	5/2007	Besson	7,796,043 B2	9/2010	Euliano et al.
7,218,967 B2	5/2007	Bergelson	7,797,033 B2	9/2010	D'Andrea et al.
7,231,451 B2	6/2007	Law	7,809,399 B2	10/2010	Lu
7,243,118 B2	7/2007	Lou	7,844,341 B2	11/2010	Von Arx et al.
7,246,521 B2	7/2007	Kim	2001/0027331 A1	10/2001	Thompson
7,249,212 B2	7/2007	Do	2001/0044588 A1	11/2001	Mault
7,252,792 B2	8/2007	Perrault	2001/0051766 A1	12/2001	Gazdzinski
7,253,716 B2	8/2007	Lovoi et al.	2002/0002326 A1	1/2002	Causey et al.
7,261,690 B2	8/2007	Teller	2002/0026111 A1	2/2002	Ackerman
7,270,633 B1	9/2007	Goscha	2002/0032385 A1	3/2002	Raymond et al.
7,273,454 B2	9/2007	Raymond et al.	2002/0040278 A1	4/2002	Anuzis et al.
7,289,855 B2	10/2007	Nghiem	2002/0077620 A1	6/2002	Sweeney et al.
7,291,497 B2	11/2007	Holmes	2002/0132226 A1	9/2002	Nair
7,292,139 B2	11/2007	Mazar et al.	2002/0192159 A1	12/2002	Reitberg
7,294,105 B1	11/2007	Islam	2002/0193669 A1	12/2002	Glukhovsky
7,313,163 B2	12/2007	Liu	2002/0198470 A1	12/2002	Imran et al.
7,317,378 B2	1/2008	Jarvis et al.	2003/0017826 A1	1/2003	Fishman
7,318,808 B2	1/2008	Tarassenko et al.	2003/0023150 A1	1/2003	Yokoi et al.
7,336,929 B2	2/2008	Yasuda	2003/0028226 A1	2/2003	Thompson
7,342,895 B2	3/2008	Serpa	2003/0065536 A1	4/2003	Hansen
7,346,380 B2	3/2008	Axelgaard et al.	2003/0076179 A1	4/2003	Branch et al.
7,349,722 B2	3/2008	Witkowski et al.	2003/0083559 A1	5/2003	Thompson
7,352,998 B2	4/2008	Palin	2003/0126593 A1	7/2003	Mault
7,353,258 B2	4/2008	Washburn	2003/0130714 A1	7/2003	Nielsen et al.
7,357,891 B2	4/2008	Yang et al.	2003/0135128 A1	7/2003	Suffin et al.
7,359,674 B2	4/2008	Markki	2003/0135392 A1	7/2003	Vrijens et al.
7,366,558 B2	4/2008	Virtanen et al.	2003/0152622 A1	8/2003	Louie-Helm et al.
7,368,191 B2	5/2008	Andelman et al.	2003/0158466 A1	8/2003	Lynn et al.
7,373,196 B2	5/2008	Ryu et al.	2003/0158756 A1	8/2003	Abramson
7,375,739 B2	5/2008	Robbins	2003/0162556 A1	8/2003	Libes
			2003/0167000 A1	9/2003	Mullick et al.
			2003/0171791 A1	9/2003	KenKnight
			2003/0171898 A1	9/2003	Tarassenko et al.
			2003/0181788 A1	9/2003	Yokoi et al.

(56)

## References Cited

## U.S. PATENT DOCUMENTS

2003/0185286	A1	10/2003	Yuen	2005/0259768	A1	11/2005	Yang et al.
2003/0187337	A1	10/2003	Tarassenko et al.	2005/0261559	A1	11/2005	Mumford
2003/0187338	A1	10/2003	Say et al.	2005/0267556	A1	12/2005	Shuros et al.
2003/0195403	A1	10/2003	Berner et al.	2005/0267756	A1	12/2005	Schultz et al.
2003/0213495	A1	11/2003	Fujita et al.	2005/0277912	A1	12/2005	John
2003/0214579	A1	11/2003	Iddan	2005/0277999	A1	12/2005	Strother et al.
2003/0216622	A1	11/2003	Meron et al.	2005/0285746	A1	12/2005	Sengupta
2003/0216625	A1	11/2003	Phipps	2005/0288594	A1	12/2005	Lewkowicz et al.
2003/0216666	A1	11/2003	Ericson et al.	2006/0001496	A1	1/2006	Abrosimov et al.
2003/0216729	A1	11/2003	Marchitto	2006/0028727	A1	2/2006	Moon et al.
2004/0008123	A1	1/2004	Carrender et al.	2006/0036134	A1	2/2006	Tarassenko et al.
2004/0018476	A1	1/2004	LaDue	2006/0058602	A1	3/2006	Kwiatkowski et al.
2004/0034295	A1	2/2004	Salganicoff	2006/0061472	A1	3/2006	Lovoi et al.
2004/0049245	A1	3/2004	Gass	2006/0065713	A1	3/2006	Kingery
2004/0073095	A1	4/2004	Causey et al.	2006/0068006	A1	3/2006	Begleiter
2004/0073454	A1	4/2004	Urquhart et al.	2006/0074283	A1	4/2006	Henderson
2004/0077995	A1	4/2004	Ferek-Petric	2006/0078765	A1	4/2006	Yang et al.
2004/0082982	A1	4/2004	Gord et al.	2006/0095091	A1	5/2006	Drew
2004/0087839	A1	5/2004	Raymond et al.	2006/0095093	A1	5/2006	Bettesh et al.
2004/0092801	A1	5/2004	Drakulic	2006/0100533	A1	5/2006	Han
2004/0106859	A1	6/2004	Say et al.	2006/0109058	A1	5/2006	Keating
2004/0115517	A1	6/2004	Fukada et al.	2006/0110962	A1	5/2006	Powell
2004/0121015	A1	6/2004	Chidlaw et al.	2006/0122474	A1	6/2006	Teller
2004/0148140	A1	7/2004	Tarassenko et al.	2006/0122667	A1	6/2006	Chavan et al.
2004/0153007	A1	8/2004	Harris	2006/0136266	A1	6/2006	Tarassenko et al.
2004/0167226	A1	8/2004	Serafini	2006/0142648	A1	6/2006	Banet
2004/0167801	A1	8/2004	Say et al.	2006/0145876	A1	7/2006	Kimura
2004/0193020	A1	9/2004	Chiba	2006/0148254	A1	7/2006	McLean
2004/0193029	A1	9/2004	Glukhovskiy	2006/0149339	A1	7/2006	Burnes
2004/0193446	A1	9/2004	Mayer et al.	2006/0155174	A1	7/2006	Glukhovskiy et al.
2004/0199222	A1	10/2004	Sun et al.	2006/0155183	A1	7/2006	Kroecker
2004/0215084	A1	10/2004	Shimizu et al.	2006/0161225	A1	7/2006	Sormann et al.
2004/0218683	A1	11/2004	Batra	2006/0179949	A1	8/2006	Kim
2004/0220643	A1	11/2004	Schmidt	2006/0183993	A1	8/2006	Horn
2004/0224644	A1	11/2004	Wu	2006/0184092	A1	8/2006	Atanasoska et al.
2004/0225199	A1	11/2004	Evanyk	2006/0204738	A1	9/2006	Dubrow et al.
2004/0253304	A1	12/2004	Gross et al.	2006/0210626	A1	9/2006	Spaeder
2004/0260154	A1	12/2004	Sidelnik	2006/0216603	A1	9/2006	Choi
2005/0017841	A1	1/2005	Doi	2006/0218011	A1	9/2006	Walker
2005/0020887	A1	1/2005	Goldberg	2006/0235489	A1	10/2006	Drew
2005/0021370	A1	1/2005	Riff	2006/0243288	A1	11/2006	Kim et al.
2005/0024198	A1	2/2005	Ward	2006/0247505	A1	11/2006	Siddiqui
2005/0027205	A1	2/2005	Tarassenko et al.	2006/0253005	A1	11/2006	Drinan
2005/0038321	A1	2/2005	Fujita et al.	2006/0270346	A1	11/2006	Ibrahim
2005/0043634	A1	2/2005	Yokoi et al.	2006/0273882	A1	12/2006	Posamentier
2005/0043894	A1	2/2005	Fernandez	2006/0276702	A1	12/2006	McGinnis
2005/0054897	A1	3/2005	Hashimoto et al.	2006/0280227	A1	12/2006	Pinkney
2005/0062644	A1	3/2005	Leci	2006/0282001	A1	12/2006	Noel
2005/0065407	A1	3/2005	Nakamura et al.	2006/0289640	A1	12/2006	Mercure
2005/0070778	A1	3/2005	Lackey	2006/0293607	A1	12/2006	Alt
2005/0090753	A1	4/2005	Goor et al.	2007/0002038	A1	1/2007	Suzuki
2005/0092108	A1	5/2005	Andermo	2007/0006636	A1	1/2007	King et al.
2005/0096514	A1	5/2005	Starkebaum	2007/0008113	A1	1/2007	Spoonhower et al.
2005/0096562	A1	5/2005	Delalic et al.	2007/0016089	A1	1/2007	Fischell et al.
2005/0101843	A1	5/2005	Quinn	2007/0027386	A1	2/2007	Such
2005/0101872	A1	5/2005	Sattler	2007/0027388	A1	2/2007	Chou
2005/0115561	A1	6/2005	Stahmann et al.	2007/0038054	A1	2/2007	Zhou
2005/0116820	A1	6/2005	Goldreich	2007/0049339	A1	3/2007	Barak et al.
2005/0117389	A1	6/2005	Worledge	2007/0055098	A1	3/2007	Shimizu et al.
2005/0121322	A1	6/2005	Say et al.	2007/0060797	A1	3/2007	Ball
2005/0131281	A1	6/2005	Ayer et al.	2007/0060800	A1	3/2007	Drinan et al.
2005/0143623	A1	6/2005	Kojima	2007/0073353	A1	3/2007	Rooney et al.
2005/0148883	A1	7/2005	Boesen	2007/0096765	A1	5/2007	Kagan
2005/0154428	A1	7/2005	Bruinsma	2007/0106346	A1	5/2007	Bergelson
2005/0156709	A1	7/2005	Gilbert et al.	2007/0123772	A1	5/2007	Euliano
2005/0165323	A1	7/2005	Montgomery	2007/0129622	A1	6/2007	Bourget
2005/0177069	A1	8/2005	Takizawa	2007/0130287	A1	6/2007	Kumar
2005/0182389	A1	8/2005	LaPorte	2007/0135803	A1	6/2007	Belson
2005/0187789	A1	8/2005	Hatlestad et al.	2007/0142721	A1	6/2007	Berner et al.
2005/0192489	A1	9/2005	Marshall	2007/0156016	A1	7/2007	Betesh
2005/0197680	A1	9/2005	DelMain et al.	2007/0162089	A1	7/2007	Mosesov
2005/0228268	A1	10/2005	Cole	2007/0162090	A1	7/2007	Penner
2005/0234307	A1	10/2005	Heinonen	2007/0167495	A1	7/2007	Brown et al.
2005/0240305	A1	10/2005	Bogash et al.	2007/0167848	A1	7/2007	Kuo et al.
2005/0245794	A1	11/2005	Dinsmoor	2007/0173701	A1	7/2007	Al-Ali
				2007/0179347	A1	8/2007	Tarassenko et al.
				2007/0179371	A1	8/2007	Peysner et al.
				2007/0185393	A1	8/2007	Zhou
				2007/0191002	A1	8/2007	Ge

(56)

## References Cited

## U.S. PATENT DOCUMENTS

2007/0196456 A1	8/2007	Stevens	2009/0030297 A1	1/2009	Miller
2007/0207793 A1	9/2007	Myer	2009/0034209 A1	2/2009	Joo
2007/0208233 A1	9/2007	Kovacs	2009/0043171 A1	2/2009	Rule
2007/0213659 A1	9/2007	Trovato et al.	2009/0048498 A1	2/2009	Riskey
2007/0237719 A1	10/2007	Jones	2009/0062634 A1	3/2009	Say et al.
2007/0244370 A1	10/2007	Kuo et al.	2009/0062670 A1	3/2009	Sterling
2007/0255198 A1	11/2007	Leong et al.	2009/0069642 A1	3/2009	Gao
2007/0255330 A1	11/2007	Lee	2009/0069655 A1	3/2009	Say et al.
2007/0270672 A1	11/2007	Hayter	2009/0069656 A1	3/2009	Say et al.
2007/0279217 A1	12/2007	Venkatraman	2009/0069657 A1	3/2009	Say et al.
2007/0282174 A1	12/2007	Sabatino	2009/0069658 A1	3/2009	Say et al.
2007/0282177 A1	12/2007	Pilz	2009/0076343 A1	3/2009	James
2007/0299480 A1	12/2007	Hill	2009/0082645 A1	3/2009	Hafezi et al.
2008/0014866 A1	1/2008	Lipowshi	2009/0087483 A1	4/2009	Sison
2008/0020037 A1	1/2008	Robertson et al.	2009/0088618 A1	4/2009	Ameson
2008/0021519 A1	1/2008	DeGeest	2009/0099435 A1	4/2009	Say et al.
2008/0021521 A1	1/2008	Shah	2009/0105561 A1	4/2009	Boyden et al.
2008/0027679 A1	1/2008	Shklarski	2009/0110148 A1	4/2009	Zhang
2008/0033273 A1	2/2008	Zhou	2009/0112626 A1	4/2009	Talbot
2008/0039700 A1*	2/2008	Drinan et al. .... 600/301	2009/0124871 A1	5/2009	Arshak
2008/0045843 A1	2/2008	Tsuji et al.	2009/0131774 A1	5/2009	Sweitzer
2008/0046038 A1	2/2008	Hill	2009/0135886 A1	5/2009	Robertson et al.
2008/0051647 A1	2/2008	Wu et al.	2009/0157113 A1	6/2009	Marcotte
2008/0051667 A1	2/2008	Goldreich	2009/0157358 A1	6/2009	Kim
2008/0058614 A1	3/2008	Banet	2009/0161602 A1	6/2009	Matsumoto
2008/0062856 A1	3/2008	Fehér	2009/0163789 A1	6/2009	Say et al.
2008/0065168 A1	3/2008	Bitton et al.	2009/0171180 A1	7/2009	Pering
2008/0074307 A1	3/2008	Boric-Lubecke	2009/0173628 A1	7/2009	Say et al.
2008/0077015 A1	3/2008	Botic-Lubecke	2009/0177055 A1	7/2009	Say et al.
2008/0077028 A1	3/2008	Schaldach et al.	2009/0177056 A1	7/2009	Say et al.
2008/0077188 A1	3/2008	Denker et al.	2009/0177057 A1	7/2009	Say et al.
2008/0091089 A1	4/2008	Guillory et al.	2009/0177058 A1	7/2009	Say et al.
2008/0091114 A1	4/2008	Min	2009/0177059 A1	7/2009	Say et al.
2008/0097549 A1	4/2008	Colbaugh	2009/0177060 A1	7/2009	Say et al.
2008/0097917 A1	4/2008	Dicks	2009/0177061 A1	7/2009	Say et al.
2008/0103440 A1	5/2008	Ferren et al.	2009/0177062 A1	7/2009	Say et al.
2008/0114224 A1	5/2008	Bandy et al.	2009/0177063 A1	7/2009	Say et al.
2008/0119705 A1	5/2008	Patel	2009/0177064 A1	7/2009	Say et al.
2008/0119716 A1	5/2008	Boric-Lubecke	2009/0177065 A1	7/2009	Say et al.
2008/0121825 A1	5/2008	Trovato et al.	2009/0177066 A1	7/2009	Say et al.
2008/0137566 A1	6/2008	Marholev	2009/0182206 A1	7/2009	Najafi
2008/0140403 A1	6/2008	Hughes et al.	2009/0182212 A1	7/2009	Say et al.
2008/0146871 A1	6/2008	Armeson et al.	2009/0182213 A1	7/2009	Say et al.
2008/0146889 A1	6/2008	Young	2009/0182214 A1	7/2009	Say et al.
2008/0146892 A1	6/2008	LeBoeuf	2009/0182215 A1	7/2009	Say et al.
2008/0154104 A1	6/2008	Lamego	2009/0182388 A1	7/2009	Von Arx
2008/0166992 A1	7/2008	Ricordi	2009/0187088 A1	7/2009	Say et al.
2008/0175898 A1	7/2008	Jones et al.	2009/0187089 A1	7/2009	Say et al.
2008/0183245 A1	7/2008	Van Oort	2009/0187090 A1	7/2009	Say et al.
2008/0188837 A1	8/2008	Belsky et al.	2009/0187091 A1	7/2009	Say et al.
2008/0194912 A1	8/2008	Trovato et al.	2009/0187092 A1	7/2009	Say et al.
2008/0208009 A1	8/2008	Shklarski	2009/0187093 A1	7/2009	Say et al.
2008/0214901 A1	9/2008	Gehman	2009/0187094 A1	7/2009	Say et al.
2008/0214985 A1	9/2008	Yanaki	2009/0187095 A1	7/2009	Say et al.
2008/0243020 A1	10/2008	Chou	2009/0187381 A1	7/2009	King et al.
2008/0249360 A1	10/2008	Li	2009/0192351 A1	7/2009	Nishino
2008/0262320 A1	10/2008	Schaefer et al.	2009/0192368 A1	7/2009	Say et al.
2008/0262336 A1	10/2008	Ryu	2009/0192369 A1	7/2009	Say et al.
2008/0269664 A1	10/2008	Trovato et al.	2009/0192370 A1	7/2009	Say et al.
2008/0275312 A1	11/2008	Mosesov	2009/0192371 A1	7/2009	Say et al.
2008/0284599 A1	11/2008	Zdeblick et al.	2009/0192372 A1	7/2009	Say et al.
2008/0288027 A1	11/2008	Kroll	2009/0192373 A1	7/2009	Say et al.
2008/0294020 A1	11/2008	Sapounas	2009/0192374 A1	7/2009	Say et al.
2008/0300572 A1	12/2008	Rankers	2009/0192375 A1	7/2009	Say et al.
2008/0303638 A1	12/2008	Nguyen	2009/0192376 A1	7/2009	Say et al.
2008/0306357 A1	12/2008	Korman	2009/0192377 A1	7/2009	Say et al.
2008/0306359 A1	12/2008	Zdeblick et al.	2009/0192378 A1	7/2009	Say et al.
2008/0306360 A1	12/2008	Robertson et al.	2009/0192379 A1	7/2009	Say et al.
2008/0311852 A1	12/2008	Hansen	2009/0198115 A1	8/2009	Say et al.
2008/0312522 A1	12/2008	Rowlandson	2009/0198116 A1	8/2009	Say et al.
2008/0316020 A1	12/2008	Robertson	2009/0198175 A1	8/2009	Say et al.
2009/0009330 A1	1/2009	Sakama et al.	2009/0203964 A1	8/2009	Shimizu et al.
2009/0009332 A1	1/2009	Nunez et al.	2009/0203971 A1	8/2009	Sciarappa
2009/0024045 A1	1/2009	Prakash	2009/0203972 A1	8/2009	Heneghan
2009/0030293 A1	1/2009	Cooper et al.	2009/0203978 A1	8/2009	Say et al.
			2009/0204265 A1	8/2009	Hackett
			2009/0210164 A1	8/2009	Say et al.
			2009/0216101 A1	8/2009	Say et al.
			2009/0216102 A1	8/2009	Say et al.

(56)

## References Cited

## U.S. PATENT DOCUMENTS

2009/0227204 A1 9/2009 Robertson et al.  
 2009/0227876 A1 9/2009 Tran  
 2009/0227940 A1 9/2009 Say et al.  
 2009/0227941 A1 9/2009 Say et al.  
 2009/0227988 A1 9/2009 Wood et al.  
 2009/0228214 A1 9/2009 Say et al.  
 2009/0231125 A1 9/2009 Baldus  
 2009/0234200 A1 9/2009 Husheer  
 2009/0243833 A1 10/2009 Huang  
 2009/0253960 A1 10/2009 Takenaka et al.  
 2009/0256702 A1 10/2009 Robertson  
 2009/0264714 A1 10/2009 Chou  
 2009/0264964 A1 10/2009 Abrahamson  
 2009/0265186 A1 10/2009 Tarassenko et al.  
 2009/0273467 A1 11/2009 Elixmann  
 2009/0281539 A1 11/2009 Selig  
 2009/0295548 A1 12/2009 Ronkka  
 2009/0296677 A1 12/2009 Mahany  
 2009/0303920 A1 12/2009 Mahany  
 2009/0306633 A1 12/2009 Trovato et al.  
 2009/0312619 A1 12/2009 Say et al.  
 2009/0318761 A1 12/2009 Rabinovitz  
 2009/0318779 A1 12/2009 Tran  
 2009/0318783 A1 12/2009 Rohde  
 2009/0318793 A1 12/2009 Datta  
 2010/0001841 A1 1/2010 Cardullo  
 2010/0010330 A1 1/2010 Rankers  
 2010/0049004 A1 2/2010 Edman et al.  
 2010/0049006 A1 2/2010 Magar  
 2010/0049012 A1 2/2010 Dijkman et al.  
 2010/0049069 A1 2/2010 Tarassenko et al.  
 2010/0056878 A1 3/2010 Partin  
 2010/0056891 A1 3/2010 Say et al.  
 2010/0056939 A1 3/2010 Tarassenko et al.  
 2010/0057041 A1 3/2010 Hayter  
 2010/0062709 A1 3/2010 Kato  
 2010/0063438 A1 3/2010 Bengtsson  
 2010/0063841 A1 3/2010 D'Ambrosia et al.  
 2010/0069002 A1 3/2010 Rong  
 2010/0069717 A1 3/2010 Hafezi et al.  
 2010/0081894 A1 4/2010 Zdeblick et al.  
 2010/0099967 A1 4/2010 Say et al.  
 2010/0099968 A1 4/2010 Say et al.  
 2010/0099969 A1 4/2010 Say et al.  
 2010/0100077 A1 4/2010 Rush  
 2010/0100078 A1 4/2010 Say et al.  
 2010/0106001 A1 4/2010 Say et al.  
 2010/0118853 A1 5/2010 Godfrey  
 2010/0139672 A1 6/2010 Kroll et al.  
 2010/0168659 A1 7/2010 Say et al.  
 2010/0179398 A1 7/2010 Say et al.  
 2010/0185055 A1 7/2010 Robertson  
 2010/0191073 A1 7/2010 Tarassenko et al.  
 2010/0210299 A1 8/2010 Gorbachov  
 2010/0222652 A1 9/2010 Cho  
 2010/0228113 A1 9/2010 Solosko  
 2010/0234706 A1 9/2010 Gilland  
 2010/0234715 A1 9/2010 Shin  
 2010/0234914 A1 9/2010 Shen  
 2010/0239616 A1 9/2010 Hafezi et al.  
 2010/0245091 A1 9/2010 Singh  
 2010/0249881 A1 9/2010 Comdorf  
 2010/0256461 A1 10/2010 Mohamedali  
 2010/0259543 A1 10/2010 Tarassenko et al.  
 2010/0268048 A1 10/2010 Say et al.  
 2010/0268049 A1 10/2010 Say et al.  
 2010/0268050 A1 10/2010 Say et al.  
 2010/0274111 A1 10/2010 Say et al.  
 2010/0280345 A1 11/2010 Say et al.  
 2010/0280346 A1 11/2010 Say et al.  
 2010/0295694 A1 11/2010 Kauffman et al.  
 2010/0298668 A1 11/2010 Hafezi et al.  
 2010/0298730 A1 11/2010 Tarassenko et al.  
 2010/0312188 A1 12/2010 Robertson et al.  
 2010/0312580 A1 12/2010 Tarassenko et al.

2011/0009715 A1 1/2011 O'Reilly et al.  
 2011/0054265 A1 3/2011 Hafezi et al.  
 2011/0065983 A1 3/2011 Hafezi et al.  
 2011/0077660 A1 3/2011 Janik et al.  
 2011/0105864 A1 5/2011 Robertson et al.  
 2011/0124983 A1 5/2011 Kroll et al.  
 2011/0224912 A1 9/2011 Bhavaraju et al.  
 2011/0230732 A1 9/2011 Edman et al.  
 2012/0062371 A1 3/2012 Radivojevic et al.

## FOREIGN PATENT DOCUMENTS

EP 1534054 5/2005  
 EP 1702553 9/2006  
 EP 1789128 5/2007  
 EP 2143369 1/2010  
 JP 61072712 4/1986  
 JP 05-228128 9/1993  
 JP 2000-506410 5/2000  
 JP 2002263185 9/2002  
 JP 2005-073886 3/2005  
 JP 2005-087552 4/2005  
 JP 2005-304880 4/2005  
 JP 2006006377 1/2006  
 JP 2006509574 3/2006  
 JP 2007-313340 12/2007  
 KR 2006077523 7/2006  
 WO WO8802237 4/1988  
 WO WO9221307 12/1992  
 WO WO9308734 5/1993  
 WO WO9319667 10/1993  
 WO WO9739963 10/1997  
 WO WO9843537 10/1998  
 WO WO9959465 11/1999  
 WO WO0033246 6/2000  
 WO WO0147466 7/2001  
 WO WO0174011 10/2001  
 WO WO0180731 11/2001  
 WO WO0245489 6/2002  
 WO WO02058330 7/2002  
 WO WO02062276 8/2002  
 WO WO02087681 11/2002  
 WO WO03050643 6/2003  
 WO WO03068061 8/2003  
 WO WO2004014225 2/2004  
 WO WO2004019172 3/2004  
 WO WO2004039256 5/2004  
 WO WO2004066833 8/2004  
 WO WO2004066834 8/2004  
 WO WO2004066903 8/2004  
 WO WO2004068881 8/2004  
 WO WO2004109316 12/2004  
 WO WO2005011237 2/2005  
 WO WO2005020023 3/2005  
 WO WO2005024687 3/2005  
 WO WO2005047837 5/2005  
 WO WO2005051166 6/2005  
 WO WO2005110238 11/2005  
 WO WO2006021932 3/2006  
 WO WO2006027586 3/2006  
 WO WO2006055892 5/2006  
 WO WO2006055956 5/2006  
 WO WO2006075016 7/2006  
 WO WO2006100620 9/2006  
 WO WO2006116718 11/2006  
 WO WO2006127355 11/2006  
 WO WO2007001724 1/2007  
 WO WO2007001742 1/2007  
 WO WO2007013952 2/2007  
 WO WO2007014084 2/2007  
 WO WO2007014527 2/2007  
 WO WO2007021496 2/2007  
 WO WO2007027660 3/2007  
 WO WO2007028035 3/2007  
 WO WO2007036687 4/2007  
 WO WO2007036741 4/2007  
 WO WO2007036746 4/2007  
 WO WO2007040878 4/2007  
 WO WO2007067054 6/2007

(56)

## References Cited

## FOREIGN PATENT DOCUMENTS

WO	WO2007071180	6/2007
WO	WO2007096810	8/2007
WO	WO2007101141	9/2007
WO	WO2007120946	10/2007
WO	WO2007127316	11/2007
WO	WO2007127879	11/2007
WO	WO2007128165	11/2007
WO	WO2007130491	11/2007
WO	WO2007143535	12/2007
WO	WO2007149546	12/2007
WO	WO2006104843	1/2008
WO	WO2008008281	1/2008
WO	WO2008030482	3/2008
WO	WO2008052136	5/2008
WO	WO2008063626	5/2008
WO	WO2008066617	6/2008
WO	WO2008076464	6/2008
WO	WO2008089232	7/2008
WO	WO2008091683	7/2008
WO	WO2008095183	8/2008
WO	WO2008097652	8/2008
WO	WO2008101107	8/2008
WO	WO2008112577	9/2008
WO	WO2008112578	9/2008
WO	WO2008120156	10/2008
WO	WO2008133394	11/2008
WO	WO2008134185	11/2008
WO	WO2008150633	12/2008
WO	WO2009001108	12/2008
WO	WO2009006615	1/2009
WO	WO2009029453	3/2009
WO	WO2009036334	3/2009
WO	WO2009051829	4/2009
WO	WO2009051830	4/2009
WO	WO2009063377	5/2009
WO	WO2009081348	7/2009
WO	WO2009111664	9/2009
WO	WO2009146082	12/2009
WO	WO2010000085	1/2010
WO	WO2010009100	1/2010
WO	WO2010011833	1/2010
WO	WO2010019778	2/2010
WO	WO2010057049	5/2010
WO	WO2010080765	7/2010
WO	WO2010080843	7/2010
WO	WO2010107563	9/2010
WO	WO2010135516	11/2010
WO	WO2011068963	6/2011
WO	WO2011133799	10/2011
WO	WO2011159336	12/2011
WO	WO2011159337	12/2011
WO	WO2011159338	12/2011
WO	WO2011159339	12/2011

## OTHER PUBLICATIONS

Arshak et al., A Review and Adaptation of Methods of Object Tracking to Telemetry Capsules IC-Med (2007) vol. 1, No. 1, Issue 1, 12pp.

"ASGE Technology Status Evaluation Report: wireless capsule endoscopy" American Soc. For Gastrointestinal Endoscopy (2006) vol. 63, No. 4; 7 pp.

Aydin et al., "Design and implementation considerations for an advanced wireless interface in miniaturized integrated sensor Microsystems" Sch. of Eng. & Electron., Edinburgh Univ., UK; (2003); abstract.

Barrie, Heidelberg pH capsule gastric analysis. Textbook of Natural Medicine, (1992), Pizzorno, Murray & Barrie.

Bohidar et al., "Dielectric Behavior of Gelatin Solutions and Gels" Colloid Polym Sci (1998) 276:81-86.

Brock, "Smart Medicine: The Application of Auto-ID Technology to Healthcare" Auto-ID Labs (2002) <http://www.autoidlabs.org/uploads/media/MIT-AUTOID-WH-010.pdf>.

Carlson et al., "Evaluation of a non-invasive respiratory monitoring system for sleeping subjects" Physiological Measurement (1999) 20(1): 53.

Coury, L. "Conductance Measurement Part 1: Theory"; Current Separations, 18:3 (1999) p. 91-96.

Delvaux et al., "Capsule endoscopy: Technique and indications" Clinical Gastroenterology (2008) vol. 22, Issue 5, pp. 813-837.

Dhar et al., "Electroless nickel plated contacts on porous silicon" Appl. Phys. Lett. 68 (10) pp. 1392-1393 (1996).

Eldek A., "Design of double dipole antenna with enhanced usable bandwidth for wideband phased array applications" Progress in Electromagnetics Research PIER 59, 1-15 (2006).

Fawaz et al., "Enhanced Telemetry System using CP-QPSK Band-Pass Modulation Technique Suitable for Smart Pill Medical Application" IFIP IEEE Dubai Conference (2008); [http://www.asic.fh-offenburg.de/downloads/ePille/IFIP\\_IEEE\\_Dubai\\_Conference.pdf](http://www.asic.fh-offenburg.de/downloads/ePille/IFIP_IEEE_Dubai_Conference.pdf).

Ferguson et al., "Dielectric Constant Studies III Aqueous Gelatin Solutions" J. Chem. Phys. 2, 94 (1934) p. 94-98.

Furse C. M., "Dipole Antennas" J. Webster (ed). Wiley Encyclopedia of Electrical and Electronics Engineering (1999) p. 575-581.

Gagliani S. "Put Your Phone, or Skin, on Vibrate" MedGadget (2012) <http://medgadget.com/2012/03/put-your-phone-or-skin-on-vibrate.html> 8pp.

Gilson, D.R. "Molecular dynamics simulation of dipole interactions", Department of Physics, Hull University, Dec. (2002), p. 1-43.

Given Imaging, "Agile Patency Brochure" (2006) [http://www.inclino.no/documents/AgilePatencyBrochure\\_Global\\_GMB-0118-01.pdf](http://www.inclino.no/documents/AgilePatencyBrochure_Global_GMB-0118-01.pdf); 4pp.

Gonzalez-Guillaumin et al., "Ingestible capsule for impedance and pH monitoring in the esophagus" IEEE Trans Biomed Eng. (2007) 54(12): 2231-6; abstract.

Greene, "Edible RFID microchip monitor can tell if you take your medicine" Bloomberg Businessweek (2010) 2 pp.; <http://www.businessweek.com/idg/2010-03-31/edible-rfid-microchip-monitor-can-tell-if-you-take-your-medicine.html>.

Heydari et al., "Analysis of the PLL jitter due to power/ground and substrate noise"; IEEE Transactions on Circuits and Systems (2004) 51(12): 2404-16.

Hoover et al., "Rx for health: Engineers design pill that signals it has been swallowed" University of Florida News (2010) 2pp.; <http://news.ufl.edu/2010/03/31/antenna-pill-2/>.

ISFET—Ion Sensitive Field-Effect Transistor; MICROSENS S.A. pdf document. First in Office Action dated Jun. 13 (2011) for U.S. Appl. No. 12/238,345; 4pp.

Intromedic, MicroCam Innovative Capsule Endoscope Pamphlet. (2006) 8 pp (<http://www.intromedic.com/en/product/productinfo.asp>).

Juvenile Diabetes Research Foundation International (JDRF), "Artificial Pancreas Project" (2010); <http://www.artificialpancreasproject.com/>; 3 pp.

Kamada K., "Electrophoretic deposition assisted by soluble anode" Materials Letters 57 (2003) 2348-2351.

Li, P-Y, et al. "An electrochemical intraocular drug delivery device", Sensors and Actuators A 143 (2008) p. 41-48.

Lifescan, "OneTouch UltraLink™" <http://www.lifescan.com/products/meters/ultralink> (2010) 2 pp.

Mackay et al., "Radio Telemetry from within the Body" Inside Information is Revealed by Tiny Transmitters that can be Swallowed or Implanted in Man or Animal Science (1991) 1196-1202; 134; American Association for the Advancement of Science, Washington D.C.

Mackay et al., "Endoradiosonde" Nature, (1957) 1239-1240, 179 Nature Publishing Group.

McKenzie et al., "Validation of a new telemetric core temperature monitor" J. Therm. Biol. (2004) 29(7-8):605-11.

Medtronic, "CareLink Therapy Management Software for Diabetes" (2010); <https://carelink.minimed.com/patient/entry.jsp?bhcp=1>; 1 pp.

Medtronic, "Carelink™ USB" (2008) [http://www.medtronicdiabetes.com/pdf/carelink\\_usb\\_factsheet.pdf](http://www.medtronicdiabetes.com/pdf/carelink_usb_factsheet.pdf) 2pp.

Medtronic "The New MiniMed Paradigm® REAL-Time Revel™ System" (2010) <http://www.medtronicdiabetes.com/products/index.html>; 2 pp.

(56)

## References Cited

## OTHER PUBLICATIONS

- Medtronic, "Mini Med Paradigm® Revel™ Insulin Pump" (2010) <http://www.medtronicdiabetes.com/products/insulinpumps/index.html>; 2 pp.
- Medtronic, Mini Med Paradigm™ Veo™ System: Factsheet (2010). <http://www.medtronic-diabetes.com.au/downloads/Paradigm%20Veo%20Factsheet.pdf>; 4 pp.
- Melanson, "Walkers swallow RFID pills for science" Engadget (2008); <http://www.engadget.com/2008/07/29/walkers-swallow-rfid-pills-for-science/>.
- Minimitter Co. Inc. "Actiheart" Traditional 510(k) Summary. Sep. 27, 2005.
- Minimitter Co. Inc. Noninvasive technology to help your studies succeed. Mini Mitter.com Mar. 31, 2009.
- Mini Mitter Co, Inc. 510(k) Premarket Notification Mini-Logger for Diagnostic Spirometer. 9-21 (1999).
- Mini Mitter Co, Inc. 510(k) Premarket Notification for VitalSense. Apr. 22, 2004.
- Minimitter Co. Inc. VitalSense Integrated Physiological Monitoring System. Product Description. (2005).
- Minimitter Co. Inc. VitalSense Wireless Vital Signs Monitoring. Temperatures.com Mar. 31, 2009.
- Mojaverian et al., "Estimation of gastric residence time of the Heidelberg capsule in humans: effect of varying food composition" *Gastroenterology* (1985) 89:(2): 392-7.
- "New 'smart pill' to track adherence" *E-Health-Insider* (2010) [http://www.e-health-insider.com/news/5910/new\\_'smart\\_pill'\\_monitors\\_medicines](http://www.e-health-insider.com/news/5910/new_'smart_pill'_monitors_medicines).
- NPL\_AntennaBasics.pdf, Radio Antennae, <http://www.erikdeman.de/html/sail018h.htm>; (2008) 3pp.
- O'Brien et al., "The Production and Characterization of Chemically Reactive Porous Coatings of Zirconium Via Unbalanced Magnetron Sputtering" *Surface and Coatings Technology* (1996) 86-87; 200-206.
- Park, "Medtronic to Buy MiniMed for \$3.7 Billion" (2001) HomeCare; [http://homecaremag.com/mag/medical\\_medtronic\\_buy\\_minimed/](http://homecaremag.com/mag/medical_medtronic_buy_minimed/); 2 pp.
- "RFID 'pill' monitors marchers" *RFID News* (2008) <http://www.rfidnews.org/2008/07/23/rfid-pill-monitors-marchers/>.
- Rolison et al., "Electrically conductive oxide aerogels: new materials in electrochemistry" *J. Mater. Chem.* (2001) 1, 963-980.
- Roulstone, et al., "Studies on Polymer Latex Films: I. A study of latex film morphology" *Polymer International* 24 (1991) pp. 87-94.
- Sanduleanu et al., "Octave tunable, highly linear, RC-ring oscillator with differential fine-coarse tuning, quadrature outputs and amplitude control for fiber optic transceivers" (2002) *IEEE MTT-S International Microwave Symposium Digest* 545-8.
- Santini, J.T. et al., "Microchips as controlled drug delivery-devices", *Agnew. Chem. Int. Ed.* (2000), vol. 39, p. 2396-2407.
- "SensiVida minimally invasive clinical systems" Investor Presentation Oct. 2009 28pp; <http://www.sensividamedtech.com/SensiVidaGeneralOctober09.pdf>.
- Shawgo, R.S. et al. "BioMEMS from drug delivery", *Current Opinion in Solid State and Material Science* 6 (2002), p. 329-334.
- Shin et al., "A Simple Route to Metal Nanodots and Nanoporous Metal Films"; *Nano Letters*, vol. 2, No. 9 (2002) pp. 933-936.
- Shrivastava et al., "A New Platform for Bioelectronics-Electronic Pill", Cummins College, (2010).; [http://www.cumminscollege.org/downloads/electronics\\_and\\_telecommunication/Newsletters/Current%20Newsletters.pdf](http://www.cumminscollege.org/downloads/electronics_and_telecommunication/Newsletters/Current%20Newsletters.pdf); First cited in third party client search conducted by Patent Eagle Search May 18, 2010 (2010).
- "Smartlife awarded patent for knitted transducer" *Innovation in Textiles News*: <http://www.innovationintextiles.com/articles/208.php>; 2pp. (2009).
- "The SmartPill Wireless Motility Capsule" SMARTPILL, The Measure of GI Health; (2010) [http://www.smartpillcorp.com/index.cfm?pagepath=Products/The\\_SmartPill\\_Capsule&id=17814](http://www.smartpillcorp.com/index.cfm?pagepath=Products/The_SmartPill_Capsule&id=17814).
- Solanas et al., "RFID Technology for the Health Care Sector" *Recent Patents on Electrical Engineering* (2008) 1, 22-31.
- Soper, S.A. et al. "Bio-Mems Technologies and Applications", Chapter 12, "MEMS for Drug Delivery", p. 325-346 (2007).
- Swedberg, "University Team Sees Ingestible RFID Tag as a Boon to Clinical Trials" *RFID Journal* Apr. 27, 2010; <http://www.rfidjournal.com/article/view/7560/1> 3pp.
- Tajalli et al., "Improving the power-delay performance in subthreshold source-coupled logic circuits" *Integrated Circuit and System Design. Power and Timing Modeling, Optimization and Simulation*, Springer Berlin Heidelberg (2008) 21-30.
- Tatbul et al., "Confidence-based data management for personal area sensor networks" *ACM International Conference Proceeding Series* (2004) 72.
- Tierney, M.J. et al "Electroreleasing Composite Membranes for Delivery of Insulin and other Biomacromolecules", *J. Electrochem. Soc.*, vol. 137, No. 6, Jun. 1990, p. 2005-2006.
- U.S. Appl. No. 12/238,345, filed Sep. 25, 2008, Hooman et al., Non-Final Office Action mailed Jun. 13, 2011 22pp.
- Walkey, "MOSFET Structure and Processing"; 97.398\* *Physical Electronics Lecture 20*; First in Office Action dated Jun. 13, 2011 for U.S. Appl. No. 12/238,345; 24 pp.
- Watson, et al., "Determination of the relationship between the pH and conductivity of gastric juice" *Physiol Meas.* 17 (1996) pp. 21-27.
- Wongmanerod et al., "Determination of pore size distribution and surface area of thin porous silicon layers by spectroscopic ellipsometry" *Applied Surface Science* 172 (2001) 117-125.
- Xiaoming et al., "A telemedicine system for wireless home healthcare based on bluetooth and the internet" *Telemedicine Journal and e-health* (2004) 10(S2): S110-6.
- Yang et al., "Fast-switching frequency synthesizer with a discriminator-aided phase detector" *IEEE Journal of Solid-State Circuits* (2000) 35(10): 1445-52.
- Yao et al., "Low Power Digital Communication in Implantable Devices Using Volume Conduction of Biological Tissues" *Proceedings of the 28th IEEE, EMBS Annual International Conference*, Aug. 30-Sep. 3, 2006.
- Zimmerman, "Personal Area Networks: Near-field intrabody communication" *IBM Systems Journal* (1996) 35 (3-4):609-17.
- Description of ePatch Technology Platform for ECG and EMG, located at [http://www.madebydelta.com/imported/images/DELTA\\_Web/documents/ME/ePatch\\_ECG\\_EMG.pdf](http://www.madebydelta.com/imported/images/DELTA_Web/documents/ME/ePatch_ECG_EMG.pdf), Dated Sep. 2, 2010.
- Zworkin, "A Radio Pill" *Nature*, (1957) 898, 179 Nature Publishing Group.
- Jung, S. "Dissolvable 'Transient Electronics' Will Be Good for Your Body and the Environment" *MedGadget*; Oct. 1, 2012; Online website: <http://medgadget.com/2012/10/dissolvable-transient-electronics-will-be-good-for-your-body-and-the-environment.html>; downloaded Oct. 24, 2012; 4 pp.
- Trutag, Technologies, Inc., Spectral Microtags for Authentication and Anti-Counterfeiting; "Product Authentication and Brand Protection Solutions"; <http://www.trutags.com/>; downloaded Feb. 12, 2013; 1 pp.

\* cited by examiner



FIG. 1

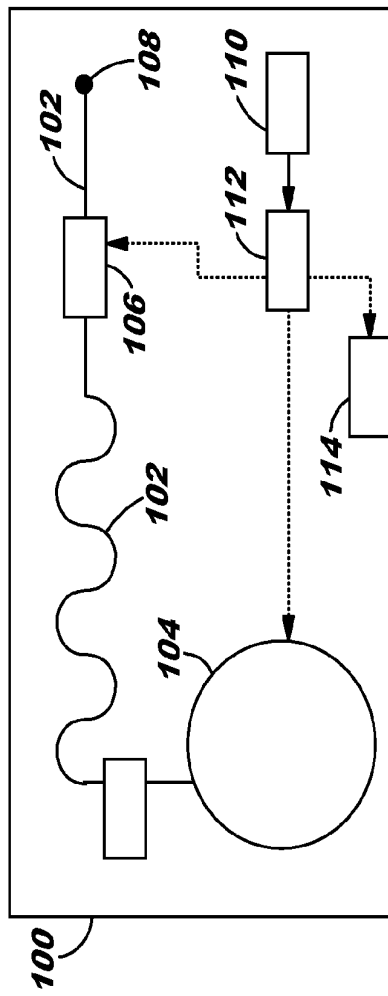


FIG. 2A

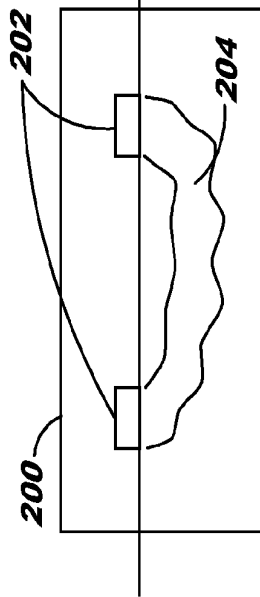


FIG. 2B


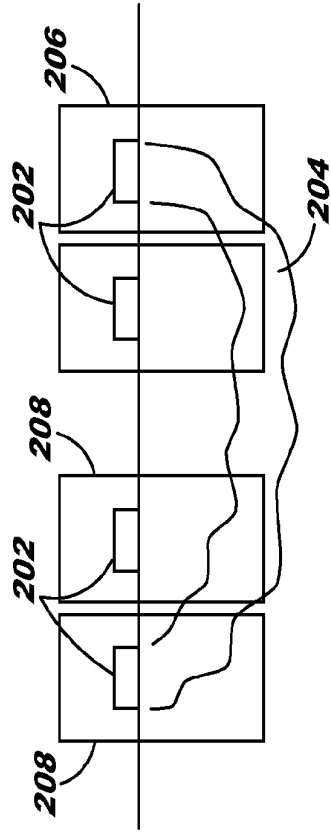


FIG. 3

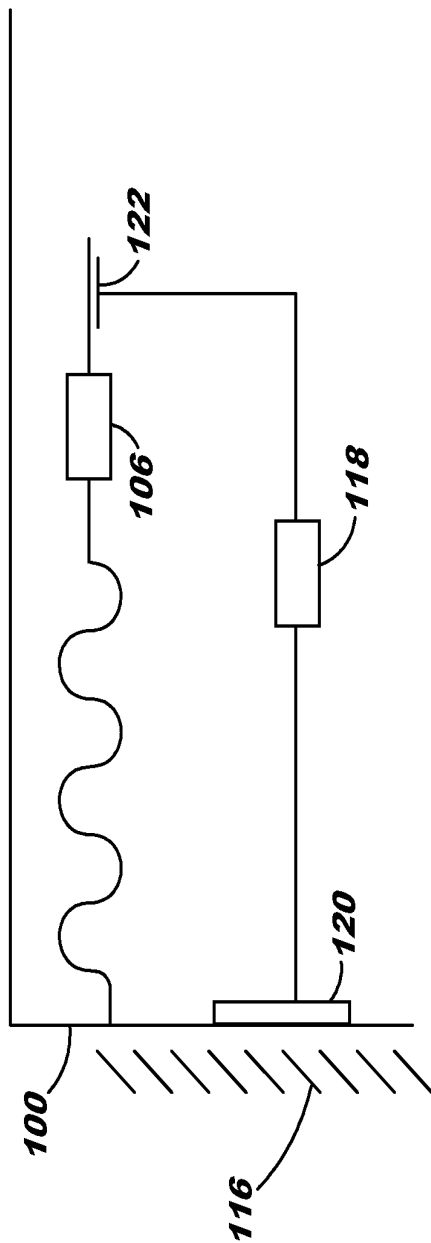

## APPARATUS AND METHOD FOR MEASURING BIOCHEMICAL PARAMETERS

### CROSS-REFERENCE TO RELATED APPLICATIONS

This application claims the benefit of U.S. application Ser. No. 61/235,979 filed Aug. 21, 2009, which application is incorporated herein by reference for all purposes.

### BACKGROUND

Microfluidic technology and other techniques may be employed to measure various types of physiologic parameters that might be important to diagnose or manage a disease.

Generally, the term “microfluidics” refers to the art making very small channels using microlithographic and microfabrication techniques. For example, a substrate such as glass with polymers may be used to make channels. Other substances used in formulating substrates include, for example, silicon and aluminum. Various other types of substrates are possible. The channels may be fabricated using various techniques, e.g., by etching silicon using a deep reactive ion etch with a mask that provides precise control of geometry. Various patterns may be employed, e.g., curved lines, straight lines, etc.

Microfluidics may be used, *inter alia*, to perform a function such as ion chromatography or liquid chromatography to look for and measure an ion or molecule. A typical application in an ion chromatograph is introduction of a small sample liquid in a column of fluid that is otherwise neutral. Introduction, for example, may be achieved via various fluid introduction components, e.g., a pump, a microsuction component, etc.

The sample moves through the column. In some examples, a field, e.g., an electric field, is applied across the column which affects the diffusion times of the ions of the sample as the ions move through the column. The ions are detected, e.g., at the end of the column. A time of injection of the ions of the sample can be calculated based on detection, diffusion rates, and the dimensions of the column.

Information may be obtained in various ways, e.g., based on measuring electroconnectivity. In various aspects, channels are filled with different materials that modify the motion rates of different ions.

Such diagnosis or disease management by means of a microfluidic approach would be helpful if it could be done conveniently and in conjunction with other processes that might already be taking place for other reasons.

### SUMMARY OF THE INVENTION

In a first embodiment, electrodes are coupled to a surface at first, second, and third locations, the first location being further from the third location than from the second location. Impedance is measured at distinct frequencies between pairs of the electrodes. As a result, impedance is measured at differing regions below the surface, one region being deeper below the surface than the other region. In a second embodiment, a microfluidic device carries out an analysis. The analysis may be within a flexible patch adhered to a surface, or may be in a solid device implanted in a body of liquid surrounded by tissue. The analysis may involve pumping a fluid or may involve drawing an analyte electrophoretically through a microfluidic channel.

### FIGURES

FIG. 1 illustrates various components associated with a first measuring device;

FIG. 2a illustrates various components associated with a second measuring device;

FIG. 2b illustrates various components associated with multiple measuring devices; and

FIG. 3 illustrates an electrophoretic approach in a measuring device.

### DETAILED DESCRIPTION

A medical device and method for measuring physiologic parameters is provided. The medical device and method may be practiced independently and/or associated with other device(s), components, and method(s). One example of integration with a device is integration with a receiver, e.g., a receiver of RFID signals and/or conduction signals. One example of a receiver of conduction signals is an ingestible event marker receiver device, as disclosed in U.S. patent application No. 61/160,289 entitled “Body-Associated Signal Receiver” filed Mar. 13, 2009. The foregoing is hereby incorporated by reference in its entirety.

One example of such a device is a microfluidic device such as a bandage-type patch designed to be temporarily or permanently attachable to the skin or implanted into the body. Another such example is one or more removably attachable or implantable devices having electrodes for measurement of various physiologic parameters. In certain aspects, the medical device may be an independently configured device or associated, e.g., wholly or partially integrated with other device(s).

In various aspects, a version of the aforementioned technique is created on the skin where the effluent is so small it simply evaporates. A reservoir liquid that represents a control liquid such as pure water may be stored on the patch and, using a microfluidic pump, the ions are pumped through the column. A sample of a patient’s bodily fluid, such as sweat, is injected into the column. Other techniques such as microsuction, electrophoresis, etc., may be used as well.

Electrophoresis generally involves putting a voltage between the skin and the column to pull ions and other types of biological materials through the skin using electrophoresis and into the sampling column to be introduced into the chromatography column. The column may be flushed at a certain rate with a background fluid or carrier fluid, for example water, and as different ions diffuse through the fluid at a different rate, the ions are separated from one another and are collected at the distal end of the column by using electrical or optical means.

Another aspect includes application of electrophoretic voltage across the column, e.g., the length of the column, the end of the column, switched in and out, etc. For example, one segment of the column can be used to view simple diffusion to separate molecules and a valve may be used to control and/or regulate the samples or a cross-channel may be activated which takes a certain amount of material which may be further separated using, for example, electrophoresis.

Aspects may be used to perform chemical analyses, physiologic analysis, and other pursuits. Examples include analysis of sweat, urine, blood etc. In some aspects, a device utilizing microfluidic principles such as the aforescribed may be implanted, e.g., inside a bladder. Various aspects include miniaturized devices, components, subcomponents, etc., as deemed suitable for such pursuits.

In some aspects, reagent(s) may be used. Generally, such reagents react chemically with the ions in some way to change the rate of diffusion or change their rate of electro-phoretic advancement.

To illustrate, and as depicted in FIG. 1, a first measuring device **100** such as a patch device is associated with a patient. The patch device has a column **102** and may have a reservoir which may include one or more fluids and a valve for regulating intake of the sample. The reservoir may be an independent component or integrated with one or more other components, e.g., the column. As the fluids leave a column **102** at outlet **108**, they creep off the patient's skin or are released into the air and essentially evaporate because the quantities, e.g., amounts of fluids, are so low that they would be virtually non-noticeable. The sample intake is facilitated by a pump **104**. The reservoir, e.g., a serpentine column, with a valve, and other components such as the pump **104** may be micro-fabricated. The liquid goes through the reservoir and through a detector device, e.g., an array of sensors, such as detector array **106** and is discharged through an outlet **108** as described in the art of ion chromatography. Coming out the detector array **106** is the column **102**, which may empty the fluid. Typically, such a small quantity of fluid would be emptied that the fluid may be absorbed, e.g., by a material such as cotton that may be associated with the patch, and/or may evaporate over time.

The device **100** is controlled by a microcontroller **112** powered for example by electrochemical cell **110**. A wireless communications link **114** may be employed to permit the microcontroller **112** to communicate sensed information to equipment external to the device **100**. The microcontroller **112** controls the pump **104** and receives signals from the sensor **106**. Importantly, the device **100** is not powered by any equipment external to the device **100** but is self-powered. The cell **110** may be self-contained, or may get its electrolyte from surrounding liquid or moisture.

A variant is shown in FIG. 3. In FIG. 3, instead of a pump **104**, we see a power supply **118**. The power supply **118** develops an electrical potential between a region **120** of nearby tissue or liquid **116** and the far end of the column at **122**. The electrical potential draws an analyte (typically ions of interest) through the column **102** for analysis in the sensor **106**.

The chief application described herein is a patch applied to the skin. The patch receives for example perspiration from the skin and detects for example glucose. But the alternative application is to implant the device in a body of liquid surrounded by, for example, an organ wall. In such an application, the device draws fluid from the body of liquid by means of a pump and passes it by a sensor. Alternatively the device draws an analyte (such as ions of interest) electrophoretically from the body of liquid.

In various aspects, devices may be configured to make such measurements at predetermined intervals, e.g., once a day or twice a day, and at different points in time when samples are required to be taken. In various aspects, the amounts of fluid, e.g., water, may be determined by the geometry of the column. One such example is a column having a very, very small diameter. Some examples include channel diameters of 50 nanometers, 100 nanometers, 50 micrometers, 100 micrometers, etc. Other diameters are possible as well.

Other applications include identification of various substances, e.g., glucose. For example, a sample may be electrophoretically pulled from the skin into the column and then glucose may be separated from the other constituents by passing it through the diffusion column.

It also may be possible to add a reagent to the sample and look for the change, e.g., look for the products, that would be a measure of the glucose concentration, glucose oxidation, etc. For example, hydrogen peroxide may be produced that

can be measured with an electrometer. In another example, a reagent may be added to a sample to look for indications of pregnancy, etc.

Various aspects include a variety of different types of chemical analysis equipment, some or all of which may be miniaturized.

In various aspects, fluids may be sampled from various locations of the body. In one example, the fluid is sampled from within the body, e.g., using an implantable device. The implantable device may be implanted into various locations, e.g., a bladder, kidney, stomach, etc. To illustrate, the implantable device may be implanted into the bladder and sample urine to measure or identify glucose. Because glucose tends to reduce the conductivity as compared to salt, salt makes a fluid more conductive and glucose makes it less conductive. A measurement of glucose going into the bladder and the volume of the bladder may be determined by sampling of fluid associate, e.g., insert or implant a device inside the bladder. Measuring the concentration of glucose in the bladder might be a way of measuring glucose in the blood, i.e., may be a proxy for measuring glucose in the blood.

Another aspect includes a device that measures fluid content, e.g., water content of patient's skin. This approach may be similar to an approach described in U.S. patent application No. 61/160,265, entitled "Volume Sensing Device, System, and Method" and filed Mar. 13, 2009, herein incorporated by reference in its entirety. In this application, the approach may be used for measuring the amount of blood in the heart where the blood-to-tissue ratio is determined by measuring the impedance at two points at two different frequencies. A comparison of a ratio of the first impedance measurement at a point in time to the second impedance measurement at a corresponding point in time may be made to determine the blood volume-related value associated with an area located between the first tissue location and the second tissue location.

Various aspects facilitate measurement of various fluids and determinations inferred from those measurements, e.g., the moisture in skin, the level of dehydration, the amount of blood volume of the patient, etc. For example heart-failure patients may be susceptible to volume overload, insufficient hydration, and other serious issues. Measurement of various fluids and determinations inferred from those measurements may provide notice of such pending or actual condition.

Continuing with this approach, comparison of these to pure saline would result in no difference and comparison to pure tissue would result in a maximum difference. Thus, the amount of fluid in the tissue is a function of what is produced, so the ratio of those two frequencies is function of the amount of fluid in the tissue. In a typical case the tissue being studied is tissue perfused with blood.

To illustrate and with reference to FIG. 2a, a second medical device **200** includes at least two electrodes **202**, e.g., an array of electrodes. Alternatively, and with respect to FIG. 2b, each of the at least two electrodes may be associated with a multiple (respective) devices **206**, **208**. The devices may be configured variously and exhibit various form factors, e.g., two adhesive patches, each adhesive patch having one or more electrodes **202**. The amount of tissue sampled is determined by the relative position of the electrodes **202**. The bulk of the current **204** will flow between the two electrodes **202**. There may be some current that goes at a farther distance and at a greater distance into the tissue, and the depth will be related to the distance apart of the two electrodes **202**.

For example, if just the area of tissue near the surface of the skin is to be sampled, the electrodes may be positioned relatively close to each other. If sampling is directed to deeper

within the tissue, then the electrodes may be positioned relatively far apart from each other. To illustrate, if sampling is directed to the blood tissue ratio of a person's leg, one electrode may be positioned in the heel region and the other electrode may be positioned in the groin region.

A patch that attaches to the skin on the torso thus might have an array of electrodes at different spacings and, in so doing, might be able to characterize the relative amount of liquid at various depths in the skin. The two closest ones would be sampling the nearest tissues, the ones closest to the surface, and the ones spaced farthest apart would be sampling more of the in-depth tissue and looking at the tissue right there. So one could construct a simple mathematical model of the amount of fluid as a function of distance into the tissue.

One may have a two-dimensional array which may be used, among other things, to construct maps of blood-tissue ratios and start imaging or looking for various tissue types and configurations, including cysts and tumors.

Additional uses include athletic-related uses. For example, an athlete engaging in exercising, riding a bicycle, or running across a soccer field or football field may tend to dehydrate at a faster rate than an individual at rest. To monitor and guard against this condition, the fluid amount may be measured and the athlete's fluid intake may be adjusted accordingly. In addition, hydration may be monitored to ensure that the athlete does not drink too much fluid during the exercise period. In various aspects, the device may provide or trigger alert(s), e.g., audible alert to the wearer, electronic trigger to a designated device, etc. The alert may be conditioned on various predetermined parameters such as fluid level too low, too high, etc.

Further uses include monitoring multiple patients, e.g., residents in a nursing home or hospital where are a large number patients and relatively low number of nurses. Alerts may be sent, for example, to the nursing station, etc.

Another use includes monitoring an accident victim, e.g., an accident victim with a head injury, the goal being to monitor swelling, lack of fluids leading to shock, etc. Combinations of parameters can also be monitored, e.g., heart rate, heart rate variability, and fluid levels through a variable connection, dual frequency measurement. In one aspect, the medical device is configured as an implantable lead. Alternatively, the device may be configured as an external device, e.g., an adhesive patch applied over the heart region of the body to determine cardiac volume, heart rate, etc.

For dehydration applications, various aspects may be employed by desert travelers, sports players, military personnel, athletes, acupuncturists, and in agricultural pursuits, e.g., determining if steers or other animals are hydrated to a level necessary for optimum market consideration.

For various applications, e.g., application to the thorax region, multiple electrodes may be variously located on the thorax to observe changes in the region's impedance and to indicate how much blood is in the thorax as when sampled, for example, at three or four electrode contact points. A matrix may be derived from such a sampling.

Another application includes an implantable device comprising at least two electrodes for implantation into various locations, e.g., a bladder, is provided. In one example, the implantable device may measure or identify glucose. Because glucose tends to reduce the conductivity as compared to salt, salt makes a fluid more conductive and glucose makes it less conductive. A measurement of glucose going into the bladder and the volume of the bladder may be determined by putting a device inside the bladder. Measuring the concentration of

glucose in the bladder might be a way of measuring glucose in the blood, i.e., may be a proxy for measuring glucose in the blood.

The foregoing examples are illustrative in nature and not determinative of scope. One skilled in the art will recognize that various alternatives, components, configurations, and steps may be used to carry out the invention described herein.

The invention claimed is:

1. An apparatus comprising:

a first electrode coupled to a surface of a material having a depth, the first electrode coupled to the surface of the material at a first location;

a second electrode coupled to the surface of the material at a second location;

a third electrode coupled to the surface of the material at a third location;

the first location being further away from the third location than from the second location;

the apparatus further comprising sensing electronics connected with the first electrode, the second electrode, and the third electrode;

the sensing electronics disposed to measure, between the first and the second electrodes, a ratio of conductivity of a first region of the material at two differing frequencies;

the sensing electronics disposed to measure, between the first and the third electrodes, a ratio of conductivity of a second region of the material at two differing frequencies;

wherein the material is tissue perfused with blood, and wherein the second region is further in depth from the surface than the first region, and

wherein the ratios of conductivity are indicative of blood/tissue ratios.

2. The apparatus of claim 1 further characterized in that the coupling of the first electrode to the surface of the material comprises an adhesive;

the coupling of the second electrode to the surface of the material comprises an adhesive; and

the coupling of the third electrode to the surface of the material comprises an adhesive.

3. The apparatus of claim 1 further characterized in that the surface comprises skin.

4. The apparatus of claim 2 further characterized in that the surface comprises skin.

5. A method for use with apparatus comprising a first electrode, a second electrode, and a third electrode, each electrode disposed for coupling to a surface of a material having a depth, and sensing electronics disposed to measure, between pairs of electrodes, a ratio of conductivity of regions of the material at two differing frequencies; the method comprising the steps of:

coupling the first electrode to the surface of the material at a first location;

coupling the second electrode to the surface of the material at a second location;

coupling the third electrode to the surface of the material at a third location;

the first location being further away from the third location than from the second location;

by means of the sensing electronics measuring, between the first and the second electrodes, a ratio of conductivity of a first region of the material at two differing frequencies;

by means of the sensing electronics measuring, between the first and the third electrodes,

a ratio of conductivity of a second region of the material at two differing frequencies;

wherein the material is tissue perfused with blood, and wherein the second region is further in depth from the surface than the first region, and wherein the ratios of conductivity are indicative of blood/tissue ratios.

5

6. The method of claim 5 further comprising the step of communicating information indicative of the ratios by means of a wireless communications link.

7. The method of claim 5 further characterized in that the coupling of the first electrode to the surface of the material comprises use of an adhesive; the coupling of the second electrode to the surface of the material comprises use of an adhesive; and the coupling of the third electrode to the surface of the material comprises use of an adhesive.

10

15

8. The method of claim 5 further characterized in that the surface comprises skin.

9. The method of claim 7 further characterized in that the surface comprises skin.

20

\* \* \* \* \*